

<Sample Information>


Order ID :GT21022
 Name :MOG35_55
 Sequence :MEVGWYRSPFSRVVHLYRNGK
 Lot. No :GT21022-0120
 Pump A :0.1%Trifluoroacetic in 100% water
 Pump B :0.1%Trifluoroacetic in 100% acetontrile
 Total Flow :1ml/min
 Wavelength :214nm
 Analytical column type:SHIMADZU Inertsil ODS-SP(4.6*250mm*5um)

Dissolution method:15%ACN+85%H2O

Inj. Volume	Module	Action	Value
Time	Module	Action	Value
0.01	Pumps	B.Conc	2
30.00	Pumps	B.Conc	65
33.00	Pumps	B.Conc	100
38.00	Pumps	B.Conc	100
40.00	Pumps	B.Conc	2
50.00	Controiier	Stop	

<Chromatogram>

Chromatogram
mV

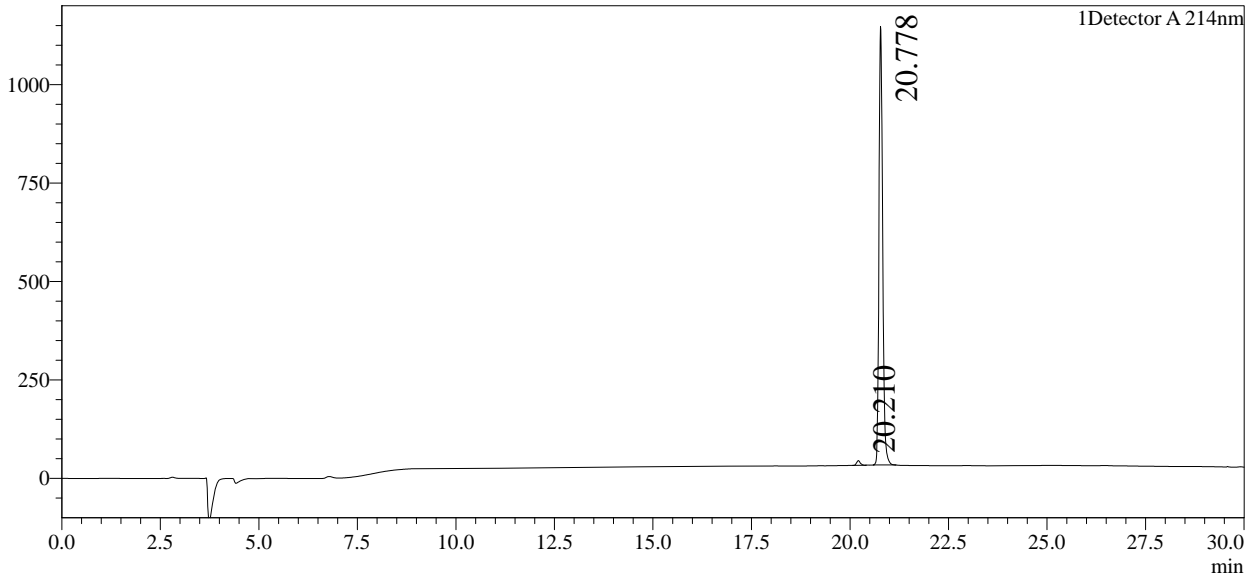

Peak Table GT21022P.lcd

Detector A 214nm

Peak#	Ret. Time	Area	Height	Area%
1	20.210	75487	11939	1.043
2	20.778	7159737	1113630	98.957
Total		7235224	1125569	100.000